

ENDOSCOPE CLEANING GUIDE


VISERA™ PEF-V Transnasal Esophagovideoscope

— Refer to companion *ENDOSCOPE DISINFECTION GUIDE* for disinfection information —

WARNING: This guide is only a summary of the steps necessary to properly clean your endoscope. Be sure to follow the detailed steps outlined in the *INSTRUCTIONS* manual that was included with your endoscope when purchased.


PRECLEANING - IMMEDIATELY AFTER USE

1

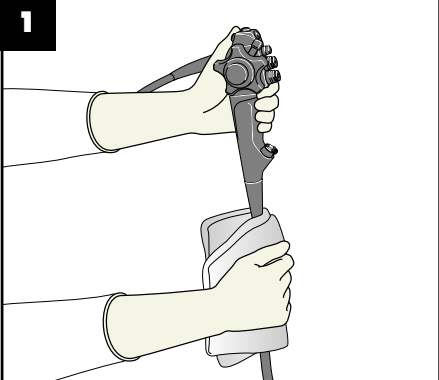


Wipe down the insertion tube with a detergent-soaked cloth.

2

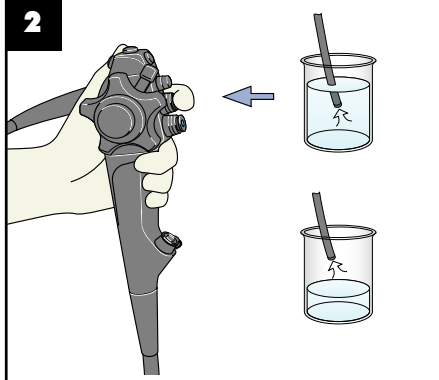


Using the suction valve, aspirate detergent, then air through suction channel.

3

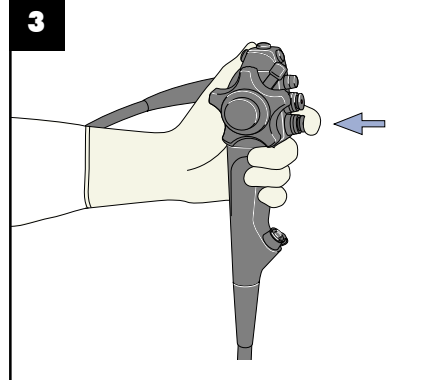

Using the air/water valve, flush water, then air, through air/water channels.

4

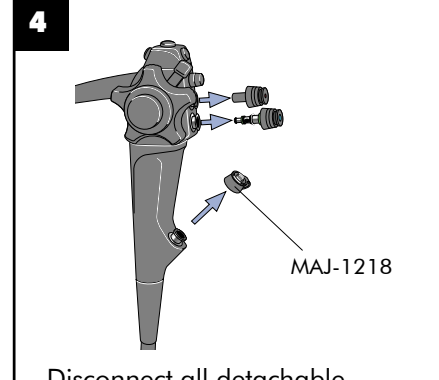


Disconnect all detachable parts and cleaning equipment. Discard single-use biopsy valve (MAJ-1218).

LEAKAGE TESTING

5


CAUTION: If a leak is detected, the endoscope must be repaired. Follow manufacturer's instructions.

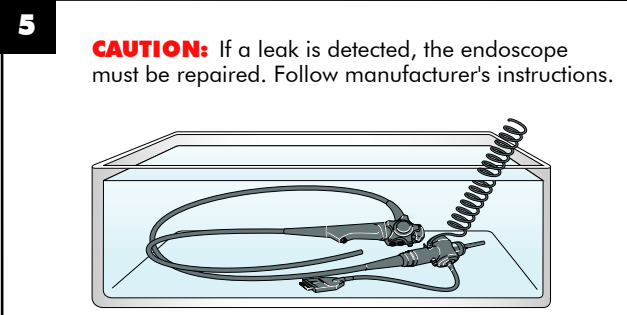

Attach leakage tester. Turn on pump. Confirm bending section has expanded. Immerse entire endoscope in clean water. Perform leakage test. Angulate tip during test. Remove from water. Detach tester after tip has deflated.


MANUAL CLEANING

6

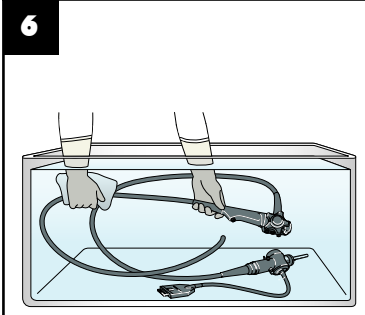


Immerse in freshly prepared detergent solution. Clean all external surfaces. Wipe endoscope distal tip.

7

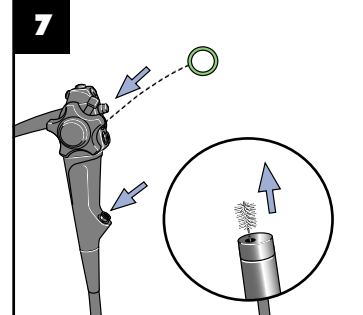


Brush the insertion tube portion of the suction channel. Repeat until all debris is removed.

8

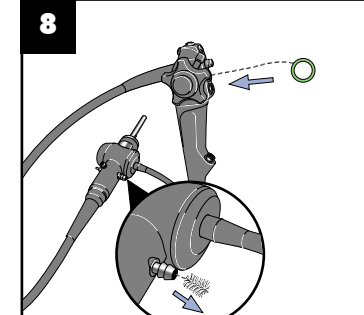


Brush the universal cord portion of the suction channel. Repeat until all debris is removed.

9

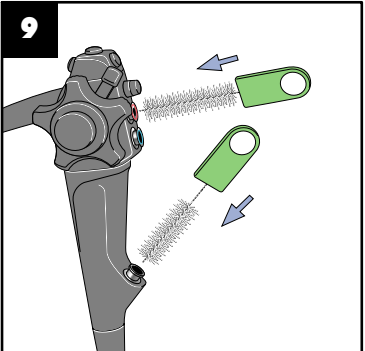


Brush the suction cylinder and instrument channel port. Repeat until all debris is removed.

10

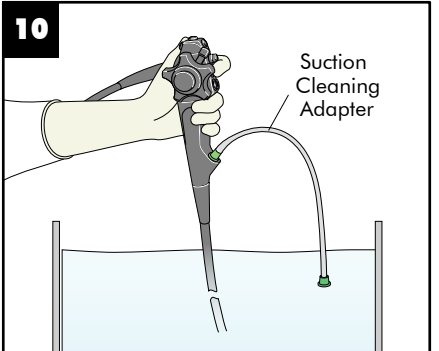


Aspirate detergent solution into suction channel.

11

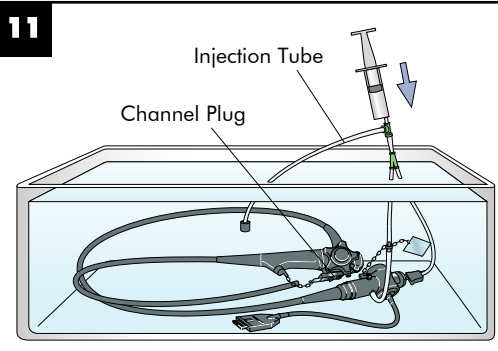

Attach injection tube & channel plug. Flush detergent solution into air, water and suction channels.


12

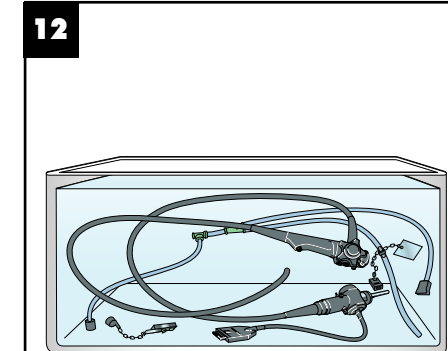

Soak in detergent solution for the time recommended by the detergent manufacturer.


RINSING

13

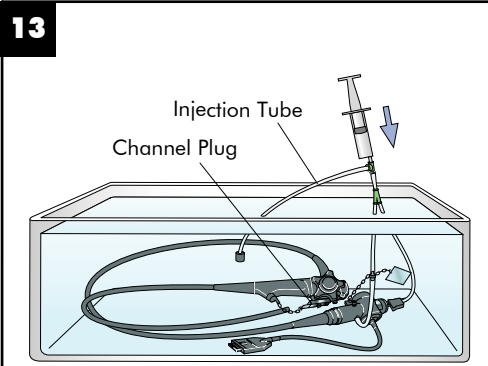


Rinse the entire instrument in clean water. Flush clean water through all channels.

14

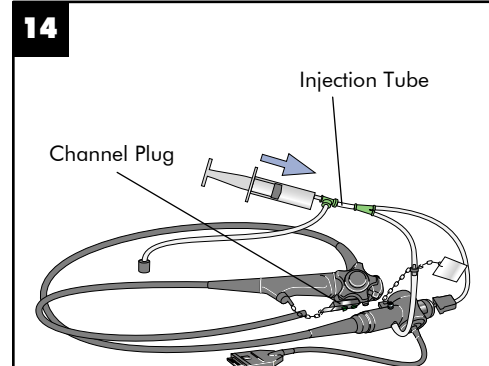

Remove from water. Flush air through all channels.

15



Use a soft, lint-free cloth to remove excess moisture from the endoscope and cleaning accessories in preparation for disinfection.

IMPORTANT

- Wear all appropriate personal protective equipment.
- Meticulous cleaning is essential for effective disinfection.
- Be sure to reprocess all removable parts (e.g., valves) according to the reprocessing manual.

Follow cleaning with appropriate high-level disinfection and alcohol-air drying.